

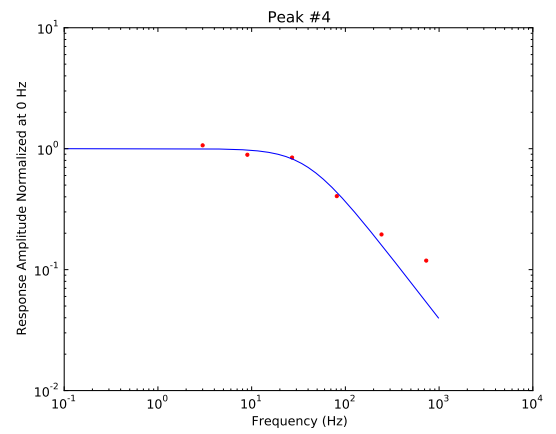
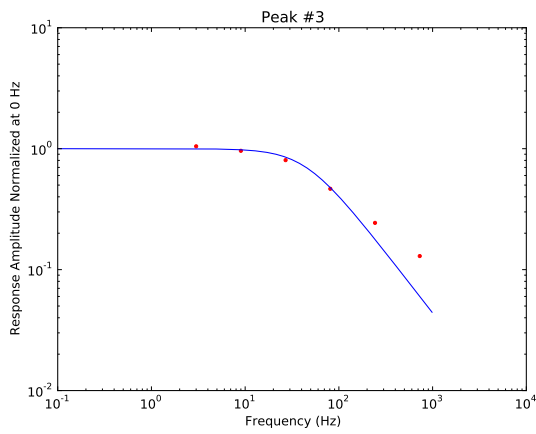
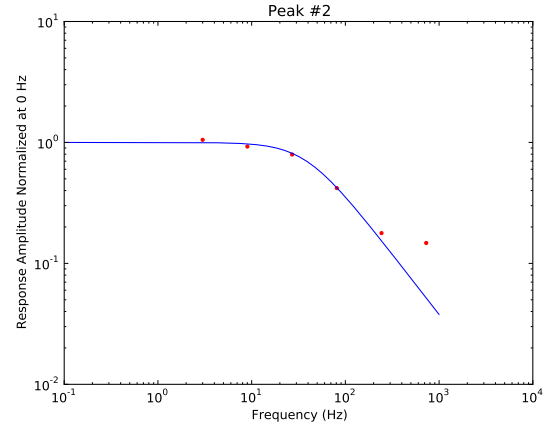
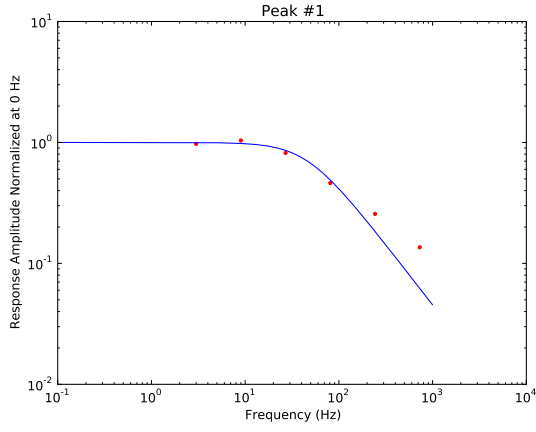
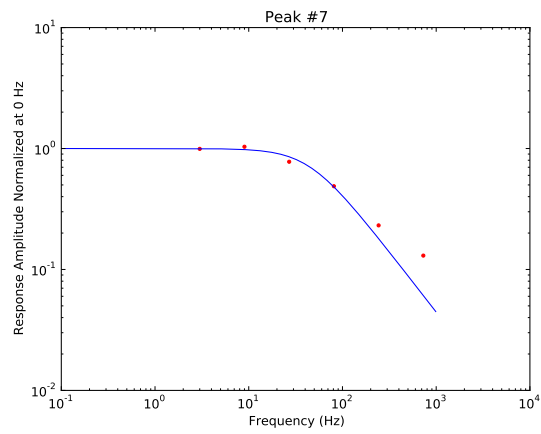


# Comb D

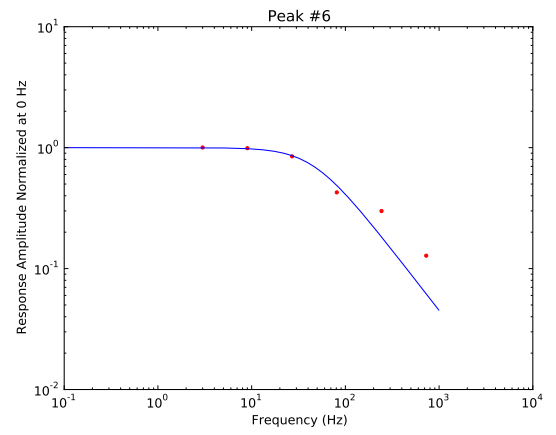

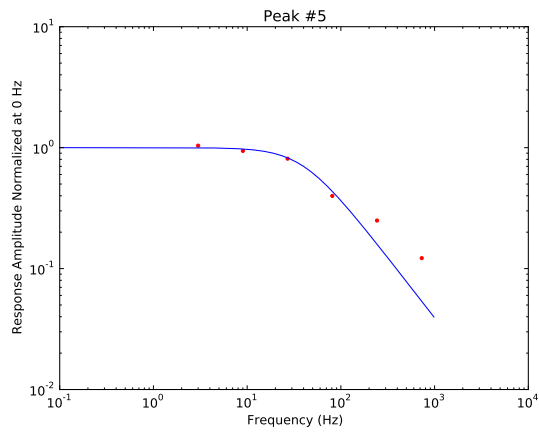

# Parameters

Table 1: Parameters for bolometer comb D

Peak ID	$\tau_{ETF}$ ms	$f_{3dB}$ Hz
1	3.51	45.31
2	4.22	37.70
3	3.64	43.77
4	4.06	39.17
5	4.07	39.09
6	3.53	45.03
7	3.59	44.34

# Distribution of electro-thermal-feedback time-constant ( $3.80 \pm 0.28 \text{ ms}$ )

